




Improving Care. Improving Business.®

## HEAVY DUTY PSYCHIATRIC RESTRAINTS

Reusable  
Non-Sterile  
Not Made with Natural Rubber Latex  
**Rx Only**

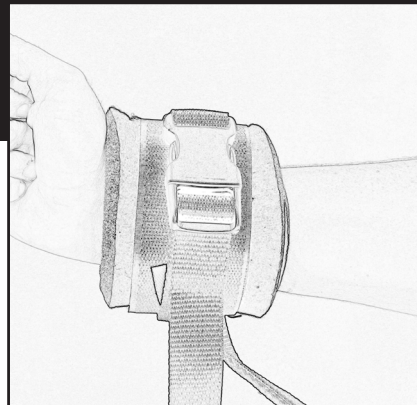

### IMPORTANT INFORMATION

Please read all instructions, warnings and precautions before use. Correct set up is essential for proper functioning of product.

This product is to be used by a licensed caregiver only for the use it was intended.

### INTENDED USE

The Heavy Duty Psychiatric Restraints are intended to be prescribed by a properly licensed practitioner to protect the patient from harming themselves, other patients, family members and/or staff.

### CONTRAINDICATIONS:

Never use on a patient if an I.V. or wound site could be compromised by the device.

### WARNINGS:

- Improper application or use of any restraint may result in serious injury or death.
- Secure straps to a portion of the bed or gurney that moves with the patient. Do not secure straps to bed or gurney side rails.
- Keep straps out of patient's reach. Patient should not be able to remove device.
- Make sure bed or gurney side rails are up while product is in use
- Check the patient regularly to ensure circulation is not compromised.

### PRECAUTIONS

This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which it is intended. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare

practitioners or healthcare providers involved in the patient's care as well as the patient. Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

Be sure to follow your facility's policies and guidelines for frequency of patient monitoring.

### INSTRUCTIONS FOR USE

1. Secure the cuffs to the patient's wrist(s) and/or ankle(s). Wrap the foam cuff around the patient's wrist(s) and ankle(s) making sure the side without the hook flap touches the patient's skin. Next, follow with the other side of the cuff making sure the hook and loop overlap securely. Finally, secure the hook flap to the loop on the cuff. Connect the male and female ends of the quick release buckle around the cuff. Pull the excess strap from the buckle to tighten.
2. Secure the straps to the bed or gurney. Take one strap and release the male and female ends of the quick release buckle. Take the strap that forms a loop from the male end of the buckle and feed it through the anchor located on the bed or gurney. Feed the male end through the loop and pull to tighten the strap around the anchor. Secure the male and female ends of the buckle. Pull the excess strap to tighten. Make sure the strap does not have slack. Apply the other strap as specified above.


Application videos can be found on [www.DeRoyal.com](http://www.DeRoyal.com).



Improving Care. Improving Business.®

## HEAVY DUTY PSYCHIATRIC RESTRAINTS

Reusable  
Non-Sterile  
Not Made with Natural Rubber Latex  
**Rx Only**

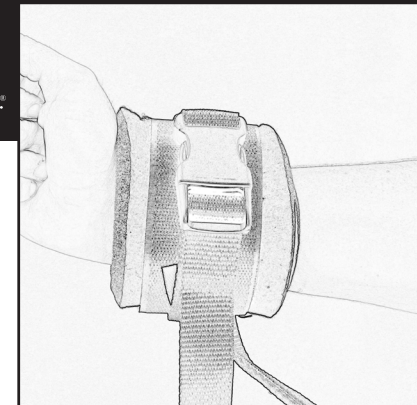

### IMPORTANT INFORMATION

Please read all instructions, warnings and precautions before use. Correct set up is essential for proper functioning of product.

This product is to be used by a licensed caregiver only for the use it was intended.

### INTENDED USE

The Heavy Duty Psychiatric Restraints are intended to be prescribed by a properly licensed practitioner to protect the patient from harming themselves, other patients, family members and/or staff.

### CONTRAINDICATIONS:

Never use on a patient if an I.V. or wound site could be compromised by the device.

### WARNINGS:

- Improper application or use of any restraint may result in serious injury or death.
- Secure straps to a portion of the bed or gurney that moves with the patient. Do not secure straps to bed or gurney side rails.
- Keep straps out of patient's reach. Patient should not be able to remove device.
- Make sure bed or gurney side rails are up while product is in use
- Check the patient regularly to ensure circulation is not compromised.

### PRECAUTIONS

This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which it is intended. The physician or practitioner is responsible for providing wearing instructions and precautions to other healthcare

practitioners or healthcare providers involved in the patient's care as well as the patient. Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or increased pain while using this product. Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

Be sure to follow your facility's policies and guidelines for frequency of patient monitoring.

### INSTRUCTIONS FOR USE

1. Secure the cuffs to the patient's wrist(s) and/or ankle(s). Wrap the foam cuff around the patient's wrist(s) and ankle(s) making sure the side without the hook flap touches the patient's skin. Next, follow with the other side of the cuff making sure the hook and loop overlap securely. Finally, secure the hook flap to the loop on the cuff. Connect the male and female ends of the quick release buckle around the cuff. Pull the excess strap from the buckle to tighten.
2. Secure the straps to the bed or gurney. Take one strap and release the male and female ends of the quick release buckle. Take the strap that forms a loop from the male end of the buckle and feed it through the anchor located on the bed or gurney. Feed the male end through the loop and pull to tighten the strap around the anchor. Secure the male and female ends of the buckle. Pull the excess strap to tighten. Make sure the strap does not have slack. Apply the other strap as specified above.

Application videos can be found on [www.DeRoyal.com](http://www.DeRoyal.com).



Improving Care. Improving Business.®

**SIZING**

**Cuff Dimensions**

14"L x 3"W

**Strap Length**

58"

**CARE INSTRUCTIONS**

To clean, hand wash with a mild fabric detergent in warm water. Do not bleach. Do not iron. Lay flat and open and allow to air dry. Inspect the product after washing to ensure it is intact. If the product is damaged, do not use it and replace it with a new one.

**WARRANTY**

DeRoyal products are warranted for one hundred twenty (120) days from the date of shipment from DeRoyal as to product quality and workmanship. DEROYAL'S WRITTEN WARRANTIES ARE GIVEN IN LIEU OF ANY IMPLIED WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.



Improving Care. Improving Business.

**Distributed by DeRoyal Industries, Inc.**

200 DeBusk Lane  
Powell, TN 37849 U.S.A.  
888.938.7828  
865.938.7828

©2014 DeRoyal Industries, Inc. All Rights Reserved.  
Part#0-1889 Revised 11/13



Improving Care. Improving Business.®

**SIZING**

**Cuff Dimensions**

14"L x 3"W

**Strap Length**

58"

**CARE INSTRUCTIONS**

To clean, hand wash with a mild fabric detergent in warm water. Do not bleach. Do not iron. Lay flat and open and allow to air dry. Inspect the product after washing to ensure it is intact. If the product is damaged, do not use it and replace it with a new one.

**WARRANTY**

DeRoyal products are warranted for one hundred twenty (120) days from the date of shipment from DeRoyal as to product quality and workmanship. DEROYAL'S WRITTEN WARRANTIES ARE GIVEN IN LIEU OF ANY IMPLIED WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.



Improving Care. Improving Business.

**Distributed by DeRoyal Industries, Inc.**

200 DeBusk Lane  
Powell, TN 37849 U.S.A.  
888.938.7828  
865.938.7828

©2014 DeRoyal Industries, Inc. All Rights Reserved.  
Part#0-1889 Revised 11/13